



**广微测**  
Gmicro Testing



中国认可  
国际互认  
检测  
TESTING  
CNAS L1747

**GUANGDONG DETECTION CENTER OF MICROBIOLOGY**

**REPORT FOR ANALYSIS**

**Report №.**

2022FM16467R01E

**Name of Sample**

AGS-MV (side 2)

**Applicant**

New Island Printing Group Co., Ltd.

**Test Type**

Entrustment Test



**Address: Building 66, No.100 Central Xian Lie Road, Guangzhou, China**

**Postcode: 510070**

**Tel: +86 20 87137666**

**Fax : +86 20 87137668**

**Website : www.gddcm.com**




GUANGDONG DETECTION CENTER OF MICROBIOLOGY

REPORT FOR ANALYSIS



Report No.: 2022FM16467R01E Verification Code: 68740951

Name of Sample	AGS-MV (side 2)	Test Type	Entrustment Test
Applicant	New Island Printing Group Co., Ltd.	Address	Room 1701, 17/F, Billion Plaza, 8 Cheung Yue Street, Cheung Sha Wan, Kowloon, Hong Kong
Sample Source	Submitted for Testing by the Applicant	Sample Quantity	12 pcs
Spec and Lot No of Sample	20220427	State and Characteristic	Paper sheet
Sample Received Date	2022-08-11	Test Completion Date	2022-09-13
Item Tested	Antiviral activity test		
Test Standard and Method	ISO 21702:2019		
Test Conclusion	The test data of the sample(s) is attached to the page(s) of this report.		
Remarks	<p>Issue Date: 2022-09-21 (Official Seal)</p> 		

Editor:

Zeng Yixiang

Verifier:

San Jia

Approver:

Xie Xiaobao



GUANGDONG DETECTION CENTER OF MICROBIOLOGY

ANALYSIS AND TEST RESULT

Report No.: 2022FM16467R01E

Virus and host cell	No.	Infectivity titre value immediate after inoculation of the reference specimen	Infectivity titre value after 24 h contacting with the reference specimen	Infectivity titre value after 24 h contacting with the test specimen
Human coronavirus (HCoV-OC43) (ATCC VR-1558) Host cell: Vero	1	5.57	4.77	<1.50
	2	5.59	4.75	<1.50
	3	5.67	4.80	<1.50
Average logarithm of infectivity titre value lgTCID <sub>50</sub> /mL		5.61	4.77	<1.50
Average logarithm of infectivity titre value lgTCID <sub>50</sub> /cm <sup>2</sup>		5.41	4.57	<1.30
Average infectivity titre value TCID <sub>50</sub> /cm <sup>2</sup> Average		2.56 × 10 <sup>5</sup>	3.71 × 10 <sup>4</sup>	<19.8
Antiviral activity value		>3.3		
Antiviral activity rate (%)		>99.9		
(Blank below)				

物分  
★  
金测专



广微测  
Gmicro Testing




中国认可  
国际互认  
检测  
TESTING  
CNAS L1747

GUANGDONG DETECTION CENTER OF MICROBIOLOGY

ANALYSIS AND TEST RESULT

Report No.: 2022FM16467R01E

Sample picture

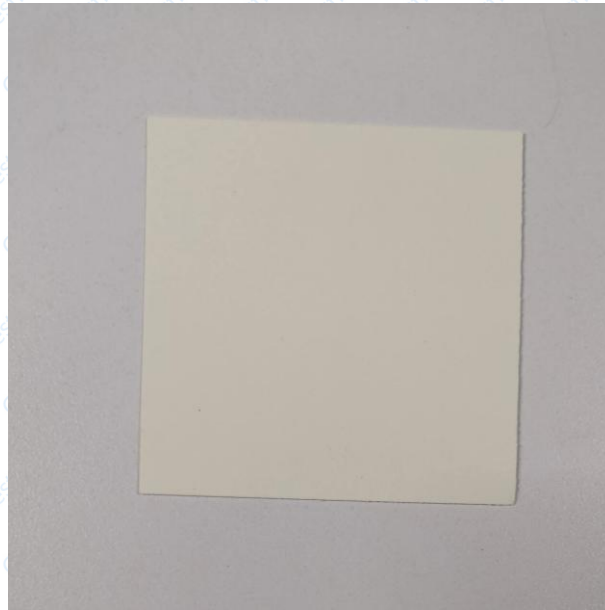



Report №.: 2022FM16467R01E

## Notice Items

1. The test report is invalid without the special stamp of testing and paging seal.
2. The test report is invalid without the signatures of the editor, the verifier and the approver.
3. The test report is invalid if being supplemented, deleted or altered.
4. Without prior written permission, the test report cannot be reproduced, except in full.
5. Unless otherwise stated, the results shown in this test report refer only to the sample(s) tested.
6. Any dispute of the test report must be raised to the testing institution within 15 days after the test report is received, exceeding which the dispute will not be accepted.
7. For the sample(s) submitted for testing, the sample information is provided by the applicant, and this testing institution is not responsible for its authenticity.

